

Journal of Biomedical Optics

SPIEDigitalLibrary.org/jbo

Errata: Monitoring of tumor response to cisplatin by subsurface fluorescence molecular tomography

Fei Liu
Xu Cao
Wei He
Jinping Song
Zhongquan Dai
Bin Zhang
Jianwen Luo
Yinghui Li
Jing Bai

Errata: Monitoring of tumor response to cisplatin by subsurface fluorescence molecular tomography

Fei Liu,^a Xu Cao,^a Wei He,^a Jinping Song,^b Zhongquan Dai,^b Bin Zhang,^a Jianwen Luo,^{a,c} Yinghui Li,^b and Jing Bai^a

^aTsinghua University, Department of Biomedical Engineering, Beijing, 100084, China

^bChina Astronaut Research and Training Center, State Key Lab of Space, Medicine Fundamentals and Application, Beijing, 100094, China

^cTsinghua University, Center for Biomedical Imaging Research, Beijing, 100084, China

[DOI: [10.1117/1.JBO.17.5.059802](https://doi.org/10.1117/1.JBO.17.5.059802)]

This article [*J. Biomed. Opt.* **17**, 040504 (2012)] was originally published online on 6 April 2012 with two errors, explained below.

Figure 1 was replaced with the figure below, in which the angles for the illumination fibers were adjusted slightly for accuracy.

Also, on p. 2, column 2, paragraph 3, the text “from 1 μm to 10 μm ” was changed to “from 1 to 10 μM .”

This article was corrected online on 20 April 2012. It appears correctly in print.

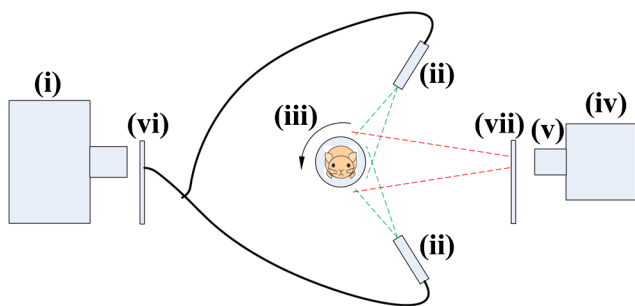


Fig. 1 Schematic top view of the noncontact full-angle subsurface FMT system.